

TEST REPORT

(Electronic version)



No: 200122326

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: NQJG-4494-34

ISSUE DATE: 2020-05-21

二维码载报告



APPLICANT: ZHONGSHAN HAOSHEN WORK SAFETY SUPPLIES & EQUIPMENTS LTD
ADDRESS: 3RD AND 4TH FLOOR, BUILDING D, NO. 5, NANYUAND ROAD, SOUTH DISTRICT, ZHONGSHAN

INFORMATION CONFIRMED BY APPLICANT:

KN95 FOLDING MASK
QUANTITY: FIFTY PIECES
COLOUR: WHITE
TYPE: HC002

DATE RECEIVED/DATE TEST STARTED: 2020-05-13

CONCLUSION:

VISUAL FIELD	M
FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER	M
INSPIRATORY RESISTANCE	M
EXPIRATORY RESISTANCE	M
FLAMMABILITY	M
HEAD BAND	M
APPEARANCE INSPECTION[2 PIECES]	M

NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT
"---" -NO COMMENT

REMARK:

THE AUTHORIZATION OF APPEARANCE INSPECTION IS NOT RECEIVED FROM CNAS.
THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200114509.
ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.
THE EXPERIMENT WAS CARRIED OUT AT No. 1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:
Yuan Liu ENGINEER

刘圆




PAGE 1 OF 4

TEST REPORT

(Electronic version)

No:200122326

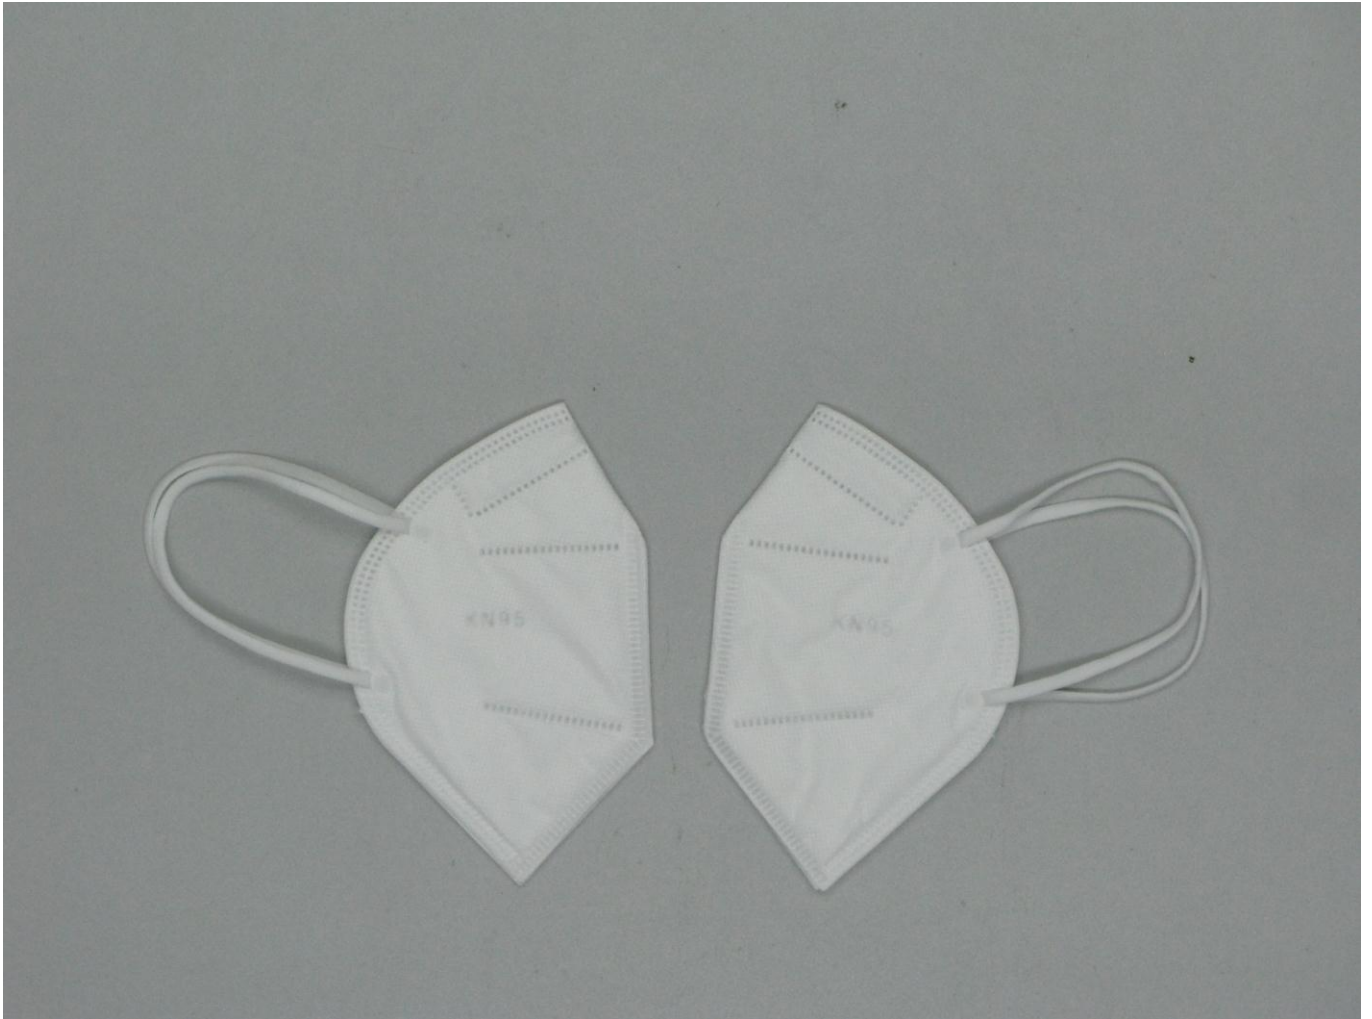

TEST REPORT

(Electronic version)

No:200122326

VISUAL FIELD(°)

(GB 2890-2009 6.8)

70

REQUIREMENT

≥60

(GB 2626-2006)

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER(%)

(GB 2626-2006 6.3, AIR FLOW:85L/min, AEROSOL:NaCl, AEROSOL CONCENTRATION:15mg/m³,
TEMP:24.3℃ RH:35.7%)

FILTRATION EFFICIENCY:

UNTREATED SAMPLE

1# 98.80

2# 98.63

3# 98.92

4# 97.68

5# 97.92

6# 99.231

7# 99.430

8# 99.425

9# 99.356

10# 98.79

CONDITIONING TREATED

1# 98.77

2# 98.53

3# 97.45

4# 99.025

5# 99.321

REQUIREMENT

FILTRATION EFFICIENCY:

≥95.0

(KN95)

(GB 2626-2006)

INSPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.5, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 151.5

2# 134.3

PRETREATMENT SAMPLE:

1# 132.2

2# 140.2

REQUIREMENT

≤350

(GB 2626-2006)

EXPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.6, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 106.0

2# 104.9

PRETREATMENT SAMPLE:

1# 95.3

2# 96.8

REQUIREMENT

≤250

(GB 2626-2006)



PAGE 3 OF 4

TEST REPORT

(Electronic version)

No:200122326

FLAMMABILITY(s)

(GB 2626-2006 6.15)

AFTERFLAME TIME
UNTREATED SAMPLE
1# 0.0
2# 0.0
CONDITIONING TREATED
3# 0.0
4# 0.0

REQUIREMENT
AFTERFLAME TIME
≤5
(GB 2626-2006)

HEAD BAND

(GB 2626-2006 6.11)

UNTREATED SAMPLE:
1# PASS
CONDITIONING TREATED:
1# PASS

REQUIREMENT
EACH HEAD BAND, BUCKLE AND OTHER ADJUST
PARTS OF MASK SHOULD NOT SLIP OR BREAK
UNDER 10N TENSION FOR 10S.
(GB 2626-2006)

APPEARANCE INSPECTION[2 PIECES]

(GB 2626-2006 6.1)

PASS

REQUIREMENT
ACCORDING TO THE CLAUSE 5.2 OF THE
PRODUCT STANDARD
(GB 2626-2006)



—End of Report—

PAGE 4 OF 4